इंटरनेट मानक

Disclosure to Promote the Right To Information

Whereas the Parliament of India has set out to provide a practical regime of right to information for citizens to secure access to information under the control of public authorities, in order to promote transparency and accountability in the working of every public authority, and whereas the attached publication of the Bureau of Indian Standards is of particular interest to the public, particularly disadvantaged communities and those engaged in the pursuit of education and knowledge, the attached public safety standard is made available to promote the timely dissemination of this information in an accurate manner to the public.

"जानने का अधिकार, जीने का अधिकार"
Mazdoor Kisan Shakti Sangathan
"The Right to Information, The Right to Live"

"पुराने को छोड नये के तरफ"
Jawaharlal Nehru
"Step Out From the Old to the New"

IS/ISO 6789 (2003): Assembly tools for screws and nuts - Hand torque tools - Requirements and test methods for design conformance testing, quality conformance testing and recalibration procedure [PGD 5: Assembly Hand Tools]

"ज्ञान से एक नये भारत का निर्माण"
Satyanarayan Gangaram Pitroda
"Invent a New India Using Knowledge"

Act Number 22 of 2005
The Indian Parliament
RIGHT TO INFORMATION

Made Available By
Public.Resource.Org

"ज्ञान एक ऐसा खजाना है जो कभी चुराया नहीं जा सकता है"
Bhartṛhari—Nītiśatakam
"Knowledge is such a treasure which cannot be stolen"

BLANK PAGE

BRUTUM FULMEN

IGNORANTIA JURIS NON EXCUSAT

PROTECTED BY COPYRIGHT

IS/ISO 6789 : 2003
(Superseding IS 7145 : 1973
and IS 7268 : 1974)

भारतीय मानक

पेंच और नट लगाने के औज़ार — हाथ के औज़ार — डिजाइन अनुरूपता परीक्षण, गुणता अनुरूपता परीक्षण और पुर्नअंशशोधन विधि की अपेक्षाएँ और परीक्षण पद्धतियाँ

Indian Standard

ASSEMBLY TOOLS FOR SCREWS AND NUTS — HAND TORQUE TOOLS — REQUIREMENTS AND TEST METHODS FOR DESIGN CONFORMANCE TESTING, QUALITY CONFORMANCE TESTING AND RECALIBRATION PROCEDURE

ICS 25.140.30

© BIS 2008

BUREAU OF INDIAN STANDARDS
MANAK BHAVAN, 9 BAHADUR SHAH ZAFAR MARG
NEW DELHI 110002

April 2008 **Price Group 7**

Assembly Hand Tools Sectional Committee, PGD 05

NATIONAL FOREWORD

This Indian Standard which is identical with ISO 6789 : 2003 'Assembly tools for screws and nuts — Hand torque tools — Requirements and test methods for design conformance testing, quality conformance testing and recalibration procedure' issued by the International Organization for Standardization (ISO) was adopted by the Bureau of Indian Standards on the recommendations of the Assembly Hand Tools Sectional Committee and approval of the Production and General Engineering Division Council

IS 7268 : 1974 'Click-type torque wrenches' was based on certain design and since then there had been substantial improvement and different types of torque wrenches have been introduced in the market. In order to align with current national and/or international manufacturing practices, the sectional committee dealing with the subject, decided to adopt ISO 6789 : 2003 as Indian Standard under dual numbering system. This Indian Standard will supersede IS 7145 : 1973 'Technical supply conditions for torque wrenches' and IS 7268 :1974 'Specification for click-type torque wrenches'.

This standard specifies the requirements and describes the test methods as well as marking of hand torque tools. The hand torque tools have been classified as indicating torque tools type and setting torque tools type.

The text of ISO Standard has been approved as suitable for publication as an Indian Standard without deviations. Certain conventions are, however, not identical to those used in Indian Standards. Attention is particularly drawn to the following:

a) Wherever the words 'International Standard' appear referring to this standard, they should be read as 'Indian Standard'.

b) Comma (,) has been used as a decimal marker, while in Indian Standards, the current practice is to use a point (.) as the decimal marker.

In this adopted standard, reference appears to the following International Standard for which Indian Standard also exists. The corresponding Indian Standard which is to be substituted in its place is listed below along with its degree of equivalence for the edition indicated:

International Standard	*Corresponding Indian Standard*	*Degree of Equivalence*
ISO 1703 : 1983[1] Assembly tools for screws and nuts — Nomenclature	IS 6293 : 1996 Assembly tools for screws and nuts — Nomenclature (*second revision*)	Technically Equivalent

The technical committee responsible for the preparation of this standard has reviewed the provisions of the following International Standard referred in this adopted standard and has decided that it is acceptable for use in conjunction with this standard:

International Standard	*Title*
ISO 1174-1 : 1996	Assembly tools for screws and nuts — Driving squares — Part 1: Driving squares for hand socket tools

The hand torque tools may also be marked with the Standard Mark. The details are given in National Annex A at the end of this standard.

For the purpose of deciding whether a particular requirement of this standard is complied with, the final value, observed or calculated, expressing the result of a test or analysis, shall be rounded off in accordance with IS 2 : 1960 'Rules for rounding off numerical values (*revised*)'. The number of significant places retained in the rounded off value should be the same as that of the specified value in this standard.

---

[1] Since revised in 2005.

Indian Standard

ASSEMBLY TOOLS FOR SCREWS AND NUTS — HAND TORQUE TOOLS — REQUIREMENTS AND TEST METHODS FOR DESIGN CONFORMANCE TESTING, QUALITY CONFORMANCE TESTING AND RECALIBRATION PROCEDURE

1 Scope

This International Standard specifies the requirements for, and describes the test methods and marking of, hand torque tools used for controlled tightening of bolted connections.

It applies to torque tools in accordance with Clause 4, in particular to indicating and setting torque wrenches in accordance with numbers 258 and 259 of ISO 1703:1983.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

GUM, *Guide for evaluation of uncertainty in measurement*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1
design conformance testing
those requirements to be met during design or modification of hand torque tools (see 5.1)

3.2
quality conformance testing
those requirements to be met during manufacture of hand torque tools (see 5.2)

3.3
calibration
set of operations that establish, under specified conditions, the relationship between values of quantities indicated by a measuring instrument or measuring system, or values represented by a material measure or a reference material, and the corresponding values realized by standards

[VIM:1993, definition 6.11]

NOTE For the specific purposes of this International Standard, the following definition may apply:

set of operations that establish, under specified conditions, the relationship between values indicated or signalled by a torque tool, and the corresponding values indicated by a calibration device

3.4
recalibration
those requirements to be met during calibration of hand torque tools after a defined period of use (see 5.3)

3.5

indicating torque tool (Type I)

tool that indicates by means of a mechanical scale, dial or electronic display, the value of torque exerted by the tool at the output drive

3.6

setting torque tool (Type II)

tool that is pre-set to a certain torque value, so that, when the prescribed value of torque is exerted by the tool at the output drive, a signal is released (e.g. audibly, visibly, perceptibly)

3.6.1

adjustable graduated torque tool (Type II, Class A, Class D and Class G)

tool designed to be adjusted by the user, which has a scale or a display to assist adjustment

3.6.2

adjustable non-graduated torque tool (Type II, Class C and Class F)

tool designed to be adjusted by the user with the aid of a calibration device

3.6.3

torque tool with fixed adjustment (Type II, Class B and Class E)

tool not designed to be adjusted by the user, i.e. having a single setting

3.7

calibration device

device used for the calibration of torque tools

4 Classification

The hand torque tools to which this International Standard applies are classified as follows:

a) Type I: Indicating torque tools (see Annex A)

- Class A: wrench, torsion or flexion bar
- Class B: wrench, rigid housing, with scale or dial or display
- Class C: wrench, rigid housing and electronic measurement
- Class D: screwdriver, with scale or dial or display
- Class E: screwdriver, with electronic measurement

b) Type II: Setting torque tools (see Annex B)

- Class A: wrench, adjustable, graduated or with display
- Class B: wrench, fixed adjustment
- Class C: wrench, adjustable, non-graduated
- Class D: screwdriver, adjustable, graduated or with display
- Class E: screwdriver, fixed adjustment
- Class F: screwdriver, adjustable, non-graduated
- Class G: wrench, flexion bar, adjustable, graduated

5 Requirements

5.1 Design conformance testing

5.1.1 General

The manufacturer shall test samples of wrenches in order to verify they are in conformity with 5.1.2 to 5.1.7.

5.1.2 Assignment of the driving square

The size of the driving square is a function of the maximum torque value of the respective torque tool. The assignment is carried out according to the values given in Table 1.

Table 1 — Assignment of the driving square

Maximum torque value N·m	Driving square nominal size[a] mm
30	6,3
135	10
340	12,5
1 000	20
2 100	25

[a] In accordance with ISO 1174-1.

5.1.3 Specified measuring range

The requirements and test methods in this International Standard cover a specified measuring range from 20 % to 100 % of the maximum torque value of the respective tool.

The scales of torque tools of Type I shall be marked with a zero position.

5.1.4 Scales

The increment between two graduation marks of a scale shall not exceed 5 % of the maximum value.

5.1.5 Tolerances

5.1.5.1 Indicating torque tools (Type I)

Permissible deviation of the torque value indicated by the tool, from the simultaneous indication of the calibration device, shall be as given in Table 2.

Table 2 — Permissible deviation (Type I)

Class[a]	Maximum torque value	
	⩽ 10 N·m	> 10 N·m
A and D	± 6 %	
B, C and E	± 6 %	± 4 %

[a] In the case of torque tools with electronic measurement (Class C and Class E) and display (Class B and Class D), the values of permissible deviation include the error due to the resolution of the display.

5.1.5.2 Setting torque tools (Type II)

Permissible deviation of the torque value set on the scale or display (Classes A, D and G) or the nominal value (Classes B and E) from the torque value indicated by the calibration device shall be as given in Table 3.

Table 3 — Permissible deviation (Type II, Classes A, B, D, E and G)

Class[a]	Maximum torque value	
	⩽ 10 N·m	> 10 N·m
A and B	± 6 %	± 4 %
D, E and G	± 6 %	

[a] In the case of torque tools with display (Class A and Class D), the values of permissible deviation include the error due to the resolution of the display.

Permissible deviation of the torque value set from the torque value indicated by the calibration device shall be as given in Table 4.

Table 4 — Permissible deviation (Type II, Classes C and F)

Class	Maximum torque value	
	⩽ 10 N·m	> 10 N·m
C	± 6 %	± 4 %
F	± 6 %	

For Classes C and F, the torque value set is equal to the arithmetical mean of the 10 test readings obtained in accordance with 6.4.

5.1.6 Overloading test

After setting at 100 % of the maximum torque value, all torque tools to be tested shall be loaded three times in each direction of operation to a torque value of 125 % of the maximum capacity (or nominal capacity for tools of Type II, Classes B and E). This does not apply to limiting torque tools.

After the overloading test, the torque tool shall still be within the tolerances specified in 5.1.5 and shall show no physical damage that can be detrimental to the torque accuracy and safety.

5.1.7 Endurance test

All torque tools to be tested shall be cycled at maximum capacity (or nominal capacity for tools of Type II, Classes B and E) for 5 000 cycles, in each direction of operation, at a rate between 5 cycles/min and 10 cycles/min.

After the endurance test, the torque tool shall still be within the tolerances specified in 5.1.5 and shall show no physical damage that can be detrimental to the torque accuracy and safety.

5.2 Quality conformance testing

All torque tools shall be tested in accordance with 6.3 and shall comply with the requirements in 5.1.5.

5.3 Recalibration

5.3.1 Method

The torque tools shall be tested in accordance with 6.3 and shall comply with the requirements in 5.1.5.

5.3.2 Interval

Torque tools shall be considered as test devices. If the user utilizes procedures for the control of test devices, torque tools shall be included in these procedures. The calibration interval shall be chosen on the basis of the factors of operation such as required accuracy, frequency of use, typical load during operation as well as ambient conditions during operation and storage conditions. The interval shall be adapted according to the procedures specified for the control of test devices and by evaluating the experience gained during recalibration.

If the user does not utilize a control procedure, a period of use of 12 months, or approximately 5 000 cycles, can be taken as a default value for the recalibration interval. For the first recalibration, the period of validity starts with user's first operation of the torque tool.

In addition to these specifications, factory or legal regulations shall be observed.

The torque tool shall be recalibrated when it has been subjected to an overload greater than the values given in 5.1.6, after repair, or after any improper handling which might influence the errors of measurement.

6 Calibration

6.1 Calibration device

The maximum permissible uncertainty of measurement of the calibration device shall be ± 1 % of the indicated value. Uncertainty of measurement shall be calculated in accordance with the "Guide for evaluation of uncertainty in measurement" (GUM), with a coverage factor $k = 2$.

The calibration device shall be set to zero before calibration is started.

6.2 Calibration temperature

The calibration shall be carried out at a temperature fluctuating by not more than ± 1 °C. This temperature shall be in the range between 18 °C to 28 °C (maximum relative humidity 90 %) and shall be documented.

6.3 Calibration conditions

6.3.1 Prior to calibration, it is to be ensured that:

a) the calibration device is oriented in accordance with Figures 1, 2 or 3;

b) for torque tools of Type I with scale or dial gauge, the direction of reading is vertical to the scale or dial gauge (parallax compensation);

c) for indicating torque tools, Type I: prior to testing in accordance with 6.4, one pre-loading up to the maximum value has been carried out in the operating direction to be tested and after release of load, the pointer or electronic indication has been set to zero. For testing in any other operating direction, this procedure shall be repeated;

d) for setting torque tools, Type II: prior to testing in accordance with 6.4, five releases without measurement have been carried out at the maximum value (nominal capacity of the torque tool) in the operating direction to be tested. For testing in any other operating direction, this procedure shall be repeated;

e) the operating force, F, is applied within the limits specified in Figures 1 and 2, in the centre of the hand hold position of the grip or the marked loading point;

f) for the torque screwdriver and T-handle torque wrenches, the operating force, T, is applied within the limits specified in Figure 3.

6.3.2 Type I torque tools shall be loaded on the calibration device with increasing force until the torque tool indicates the respective torque value. Type II setting torque tools shall be loaded on the calibration device with increasing force up to approximately 80 % of the respective target torque value. From 80 % to the final target torque value, the load shall be applied slowly and uniformly during a period of 0,5 s to 4 s.

If for Type I torque tools the torque value to be measured has been exceeded, this calibration stage shall be repeated from the zero position.

Type II torque tools, except Class B and Class E, shall be adjusted to the respective test value, starting from a lower value.

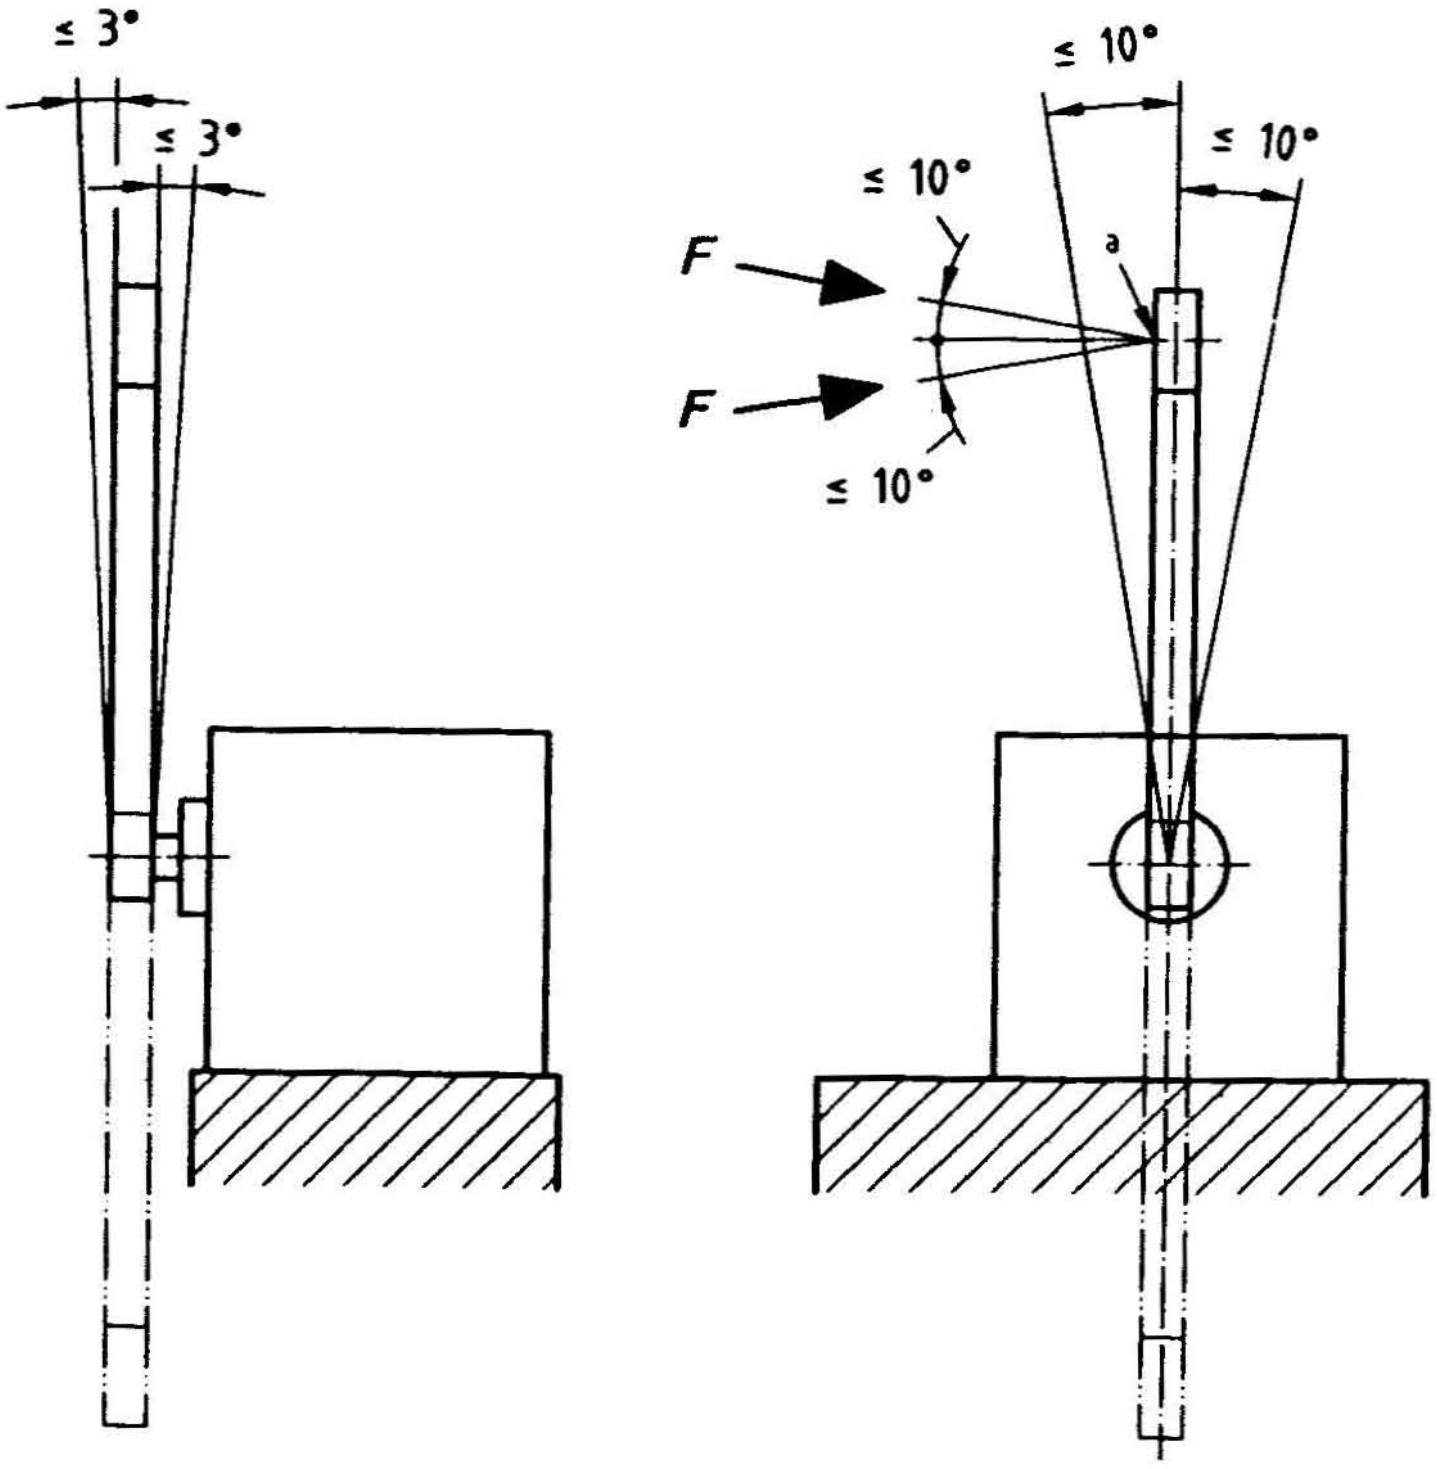

[a] Line contact, marked loading point or centre of the hand hold position of the grip.

Figure 1 — Testing of a wrench in a vertical position

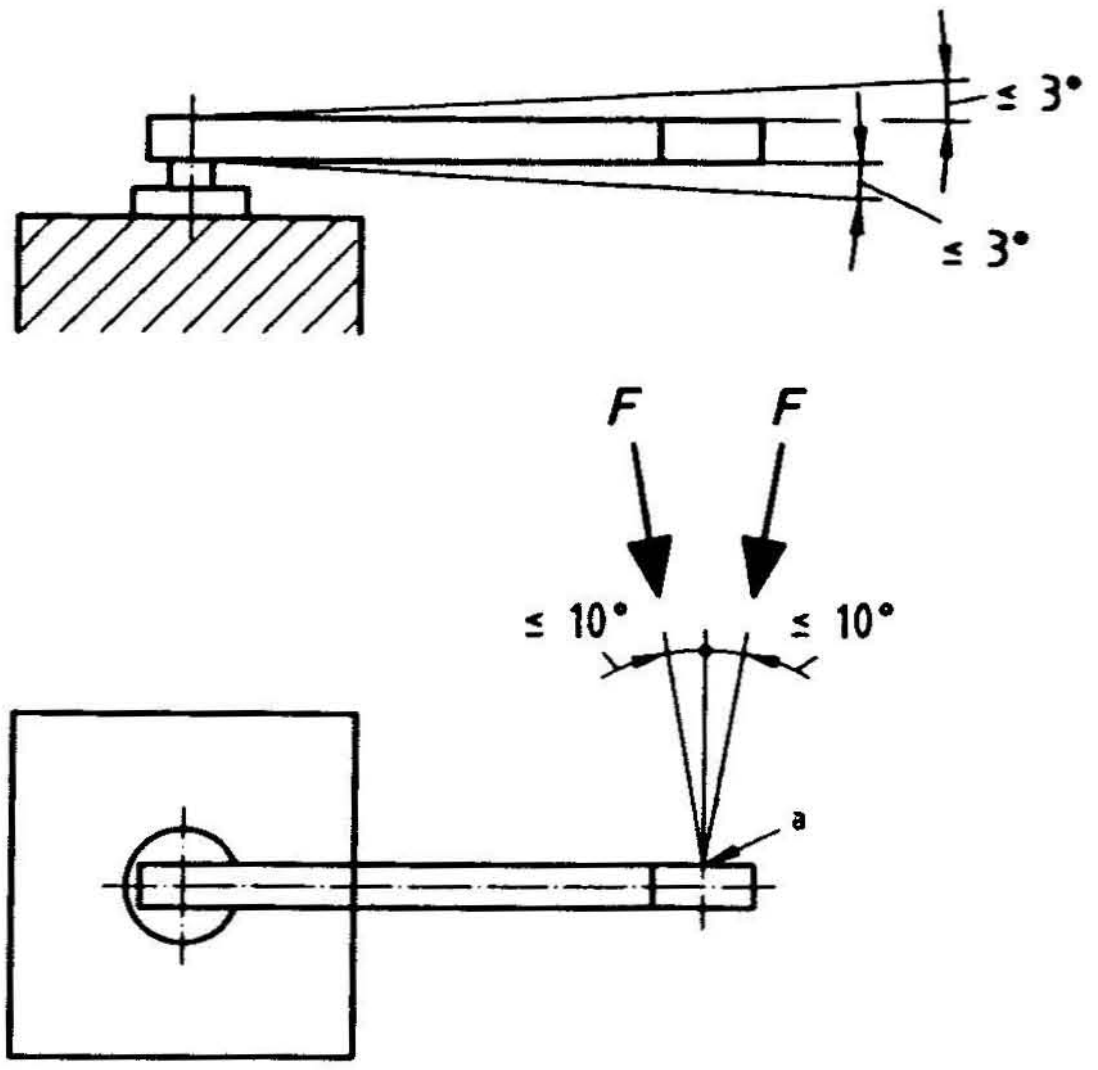

[a] Line contact, marked loading point or centre of the hand hold position of the grip.

Figure 2 — Testing of a wrench in a horizontal position

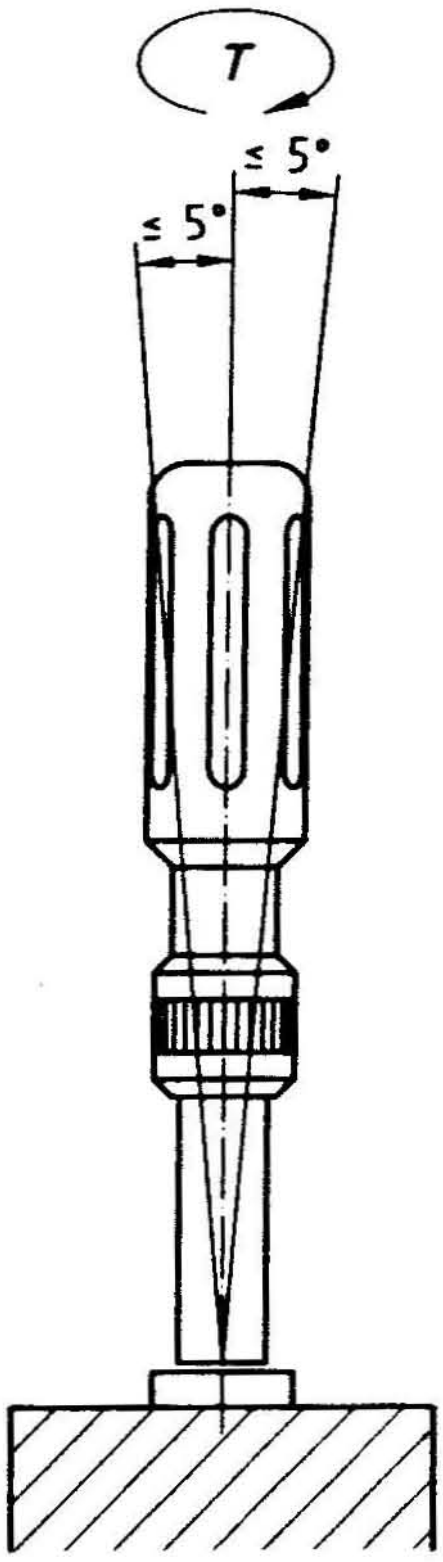

Figure 3 — Testing of a torque screwdriver and T-handle torque wrench in horizontal and vertical positions

6.4 Calibration sequence

The torque tools shall be tested first at 20 % and then at about 60 % and at 100 % of the maximum torque value of the torque tools (or at the nominal/set value for tools of Type II, Classes B and E).

If the scale mark of 20 % of the maximum torque value is not indicated on the torque tool, the permissible deviation shall be determined at the next lower scale mark.

In every operating direction, the number of measurements shall be as follows:

— Type I, all classes	5 times in a row, for every point of measurement;
— Type II, Classes A, D and G	5 times in a row, for every point of measurement;
— Type II, Classes B and E	5 times at the nominal/set value;
— Type II, Classes C and F	10 times in a row, for every point of measurement.

All readings shall be within the maximum tolerances specified in 5.1.5 and shall be recorded.

The evaluation of the deviation shall be made by the following formula:

$$A_\mathrm{s}\,(\%) = \frac{(x_\mathrm{a} - x_\mathrm{r})100}{x_\mathrm{r}}$$

where

A_s (%) is the calculated deviation of the torque tool;

x_a is the indicated value of the torque tool;

x_r is the reference value (determined by the calibration device).

6.5 Calibration examples

EXAMPLE 1 Calculation of the deviation of indicating and setting torque tools (except Type II, Class C and Class F):

- indicated value of dial, mechanical scale or display (Type I, Classes A, B, C, D and E) or
- set value of mechanical scale or display (Type II, Classes A, D and G) or
- nominal value (Type II, Classes B and E):

$X_\mathrm{a} = 100$ N·m

Reference values (determined by the calibration device)

$x_\mathrm{r1} = 104$ N·m

$x_\mathrm{r2} = 96$ N·m

$x_\mathrm{r3} = 103$ N·m

$x_\mathrm{r4} = 99$ N·m

$x_\mathrm{r5} = 101$ N·m

Calculated deviations of the torque tools in %

$$A_{s1} = \frac{(100 - 104) \times 100}{104}$$

$$A_{s1} = -3{,}85\ \%$$

$$A_{s2} = \frac{(100 - 96) \times 100}{96}$$

$$A_{s2} = 4{,}17\ \%$$

$$A_{s3} = \frac{(100 - 103) \times 100}{103}$$

$$A_{s3} = -2{,}91\ \%$$

$$A_{s4} = \frac{(100 - 99) \times 100}{99}$$

$$A_{s4} = 1{,}01\ \%$$

$$A_{s5} = \frac{(100 - 101) \times 100}{101}$$

$$A_{s5} = -0{,}99\ \%$$

EXAMPLE 2 Calculation of the deviation of setting torque tools, adjustable, non-graduated (Type II, Class C and Class F):

— Set value relevant to the arithmetical mean of the 10 reference values (determined by the calibration device)

$$x_a = \frac{x_{r1} + x_{r2} + \ldots\ldots x_{r10}}{10}$$

$$a = \frac{104 + 96 + 103 + 99 + 101 + 98 + 97 + 101 + 100{,}5 + 102{,}5}{10}$$

$$x_a = 100{,}2\ \text{N·m}$$

Reference values (determined by the calibration device)

$x_{r1} = 104$ N·m

$x_{r2} = 96$ N·m

$x_{r3} = 103$ N·m

$x_{r4} = 99$ N·m

$x_{r5} = 101$ N·m

$x_{r6} = 98$ N·m

$x_{r7} = 97$ N·m

$x_{r8} = 101$ N·m

$x_{r9} = 100{,}5$ N·m

$x_{r10} = 102{,}5$ N·m

Calculated deviations of the torque tools in %

$$A_{s1} = \frac{(100{,}2 - 104) \times 100}{104}$$

$$A_{s1} = -3{,}65\ \%$$

$$A_{s2} = \frac{(100{,}2 - 96) \times 100}{96}$$

$$A_{s2} = 4{,}38\ \%$$

$$A_{s3} = \frac{(100{,}2 - 103) \times 100}{103}$$

$$A_{s3} = -2{,}72\ \%$$

$$A_{s4} = \frac{(100{,}2 - 99) \times 100}{99}$$

$$A_{s4} = 1{,}21\ \%$$

$$A_{s5} = \frac{(100{,}2 - 101) \times 100}{101}$$

$$A_{s5} = -0{,}79\ \%$$

$$A_{s6} = \frac{(100{,}2 - 98) \times 100}{98}$$

$$A_{s6} = 2{,}24\ \%$$

$$A_{s7} = \frac{(100{,}2 - 97) \times 100}{97}$$

$$A_{s7} = 3{,}30\ \%$$

$$A_{s8} = \frac{(100{,}2 - 101) \times 100}{101}$$

$$A_{s8} = -0{,}79\ \%$$

$$A_{s9} = \frac{(100{,}2 - 100{,}5) \times 100}{100{,}5}$$

$$A_{s9} = -0{,}30\ \%$$

$$A_{s10} = \frac{(100{,}2 - 102{,}5) \times 100}{102{,}5}$$

$$A_{S10} = -2{,}24\ \%$$

7 Marking

Hand torque tools shall be marked, permanently and legibly, at least with the following information:

a) the maximum torque value;

b) the unit of measuring;

c) the direction of operation (for tools capable of operating in one direction only);

d) the name or trademark of the manufacturer (or responsible supplier);

e) where accompanied by a calibration certificate, the torque tool shall have a serial or identification number. If necessary, an identification number shall be assigned by the calibration laboratory.

Annex A
(normative)

Indicating torque tools: Type I

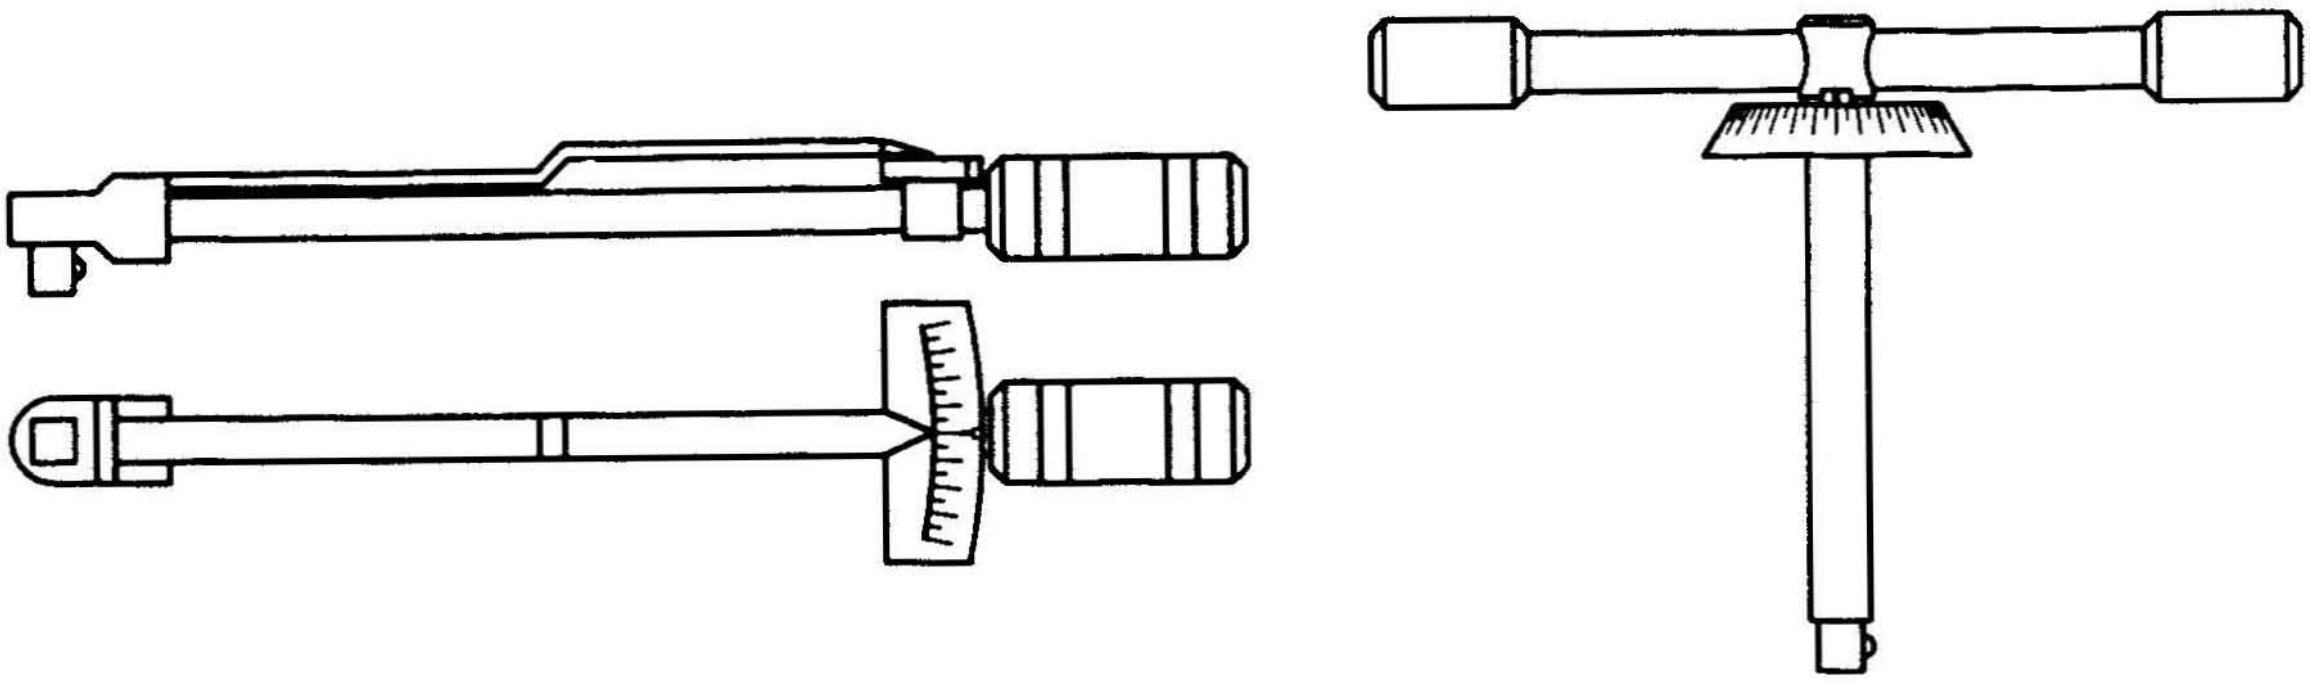

Figure A.1 — Class A: wrench, torsion or flexion bar

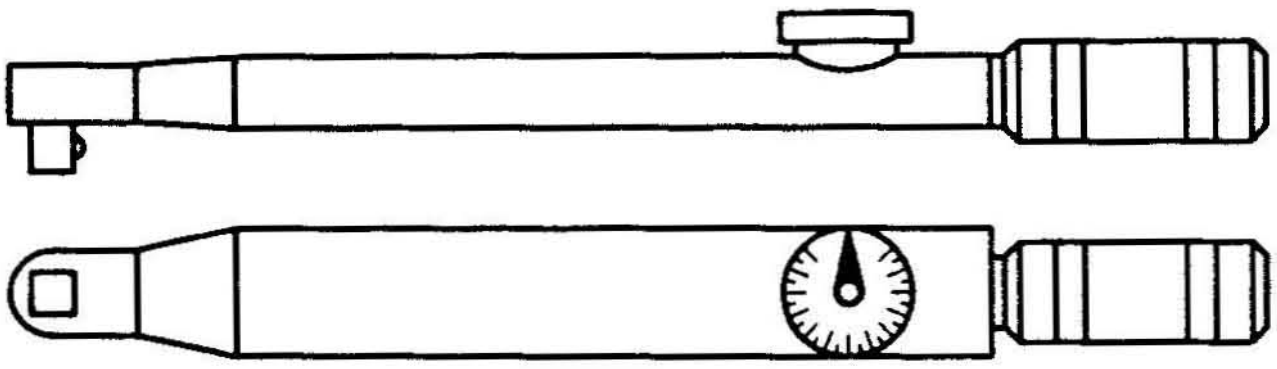

Figure A.2 — Class B: wrench, rigid housing, with scale or dial or display

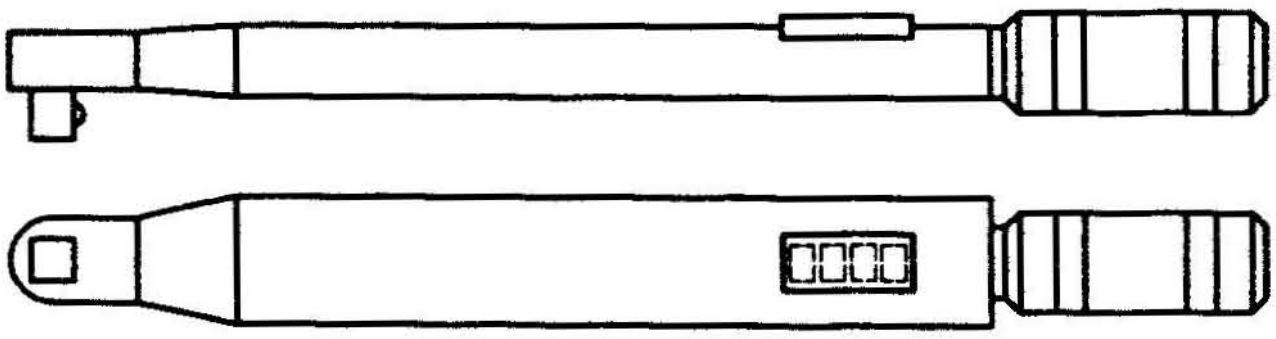

Figure A.3 — Class C: wrench, rigid housing and electronic measurement



Figure A.4 — Class D: screwdriver, with scale or dial or display



Figure A.5 — Class E: screwdriver, with electronic measurement

Annex B
(normative)

Setting torque tools: Type II

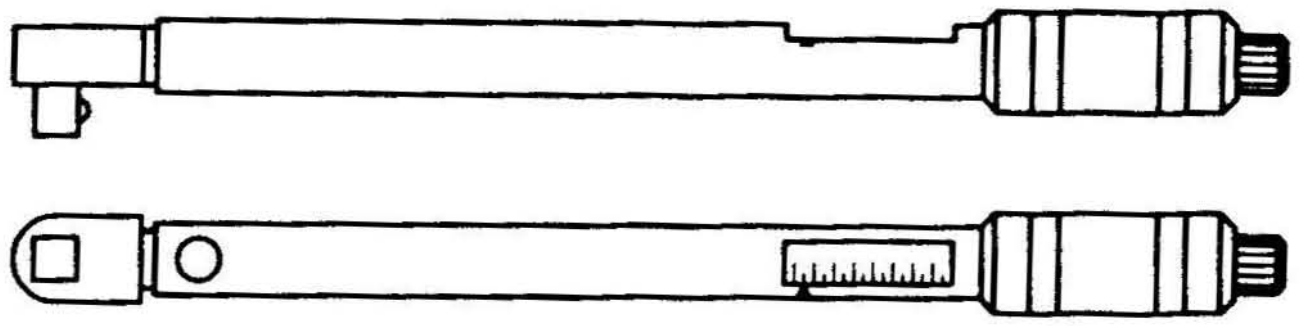

Figure B.1 — Class A: wrench, adjustable, graduated or with display

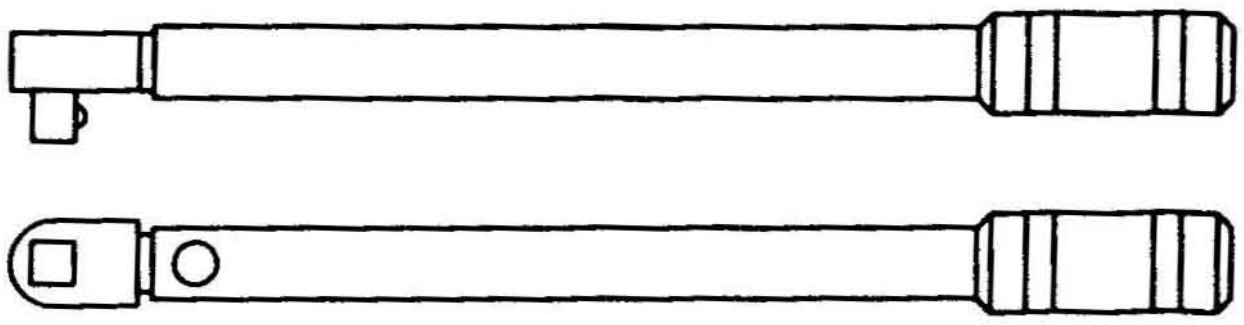

Figure B.2 — Class B: wrench, fixed adjustment

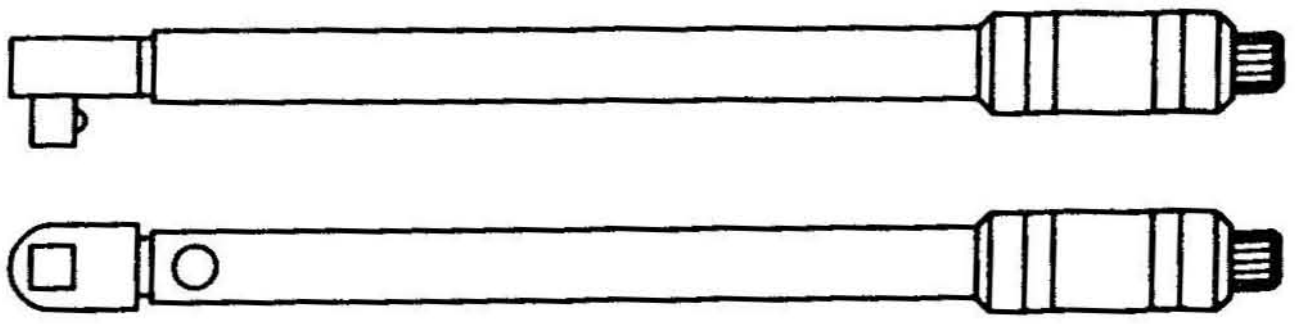

Figure B.3 — Class C: wrench, adjustable, non-graduated



Figure B.4 — Class D: screwdriver, adjustable, graduated or with display



Figure B.5 — Class E: screwdriver, fixed adjustment



Figure B.6 — Class F: screwdriver, adjustable, non-graduated

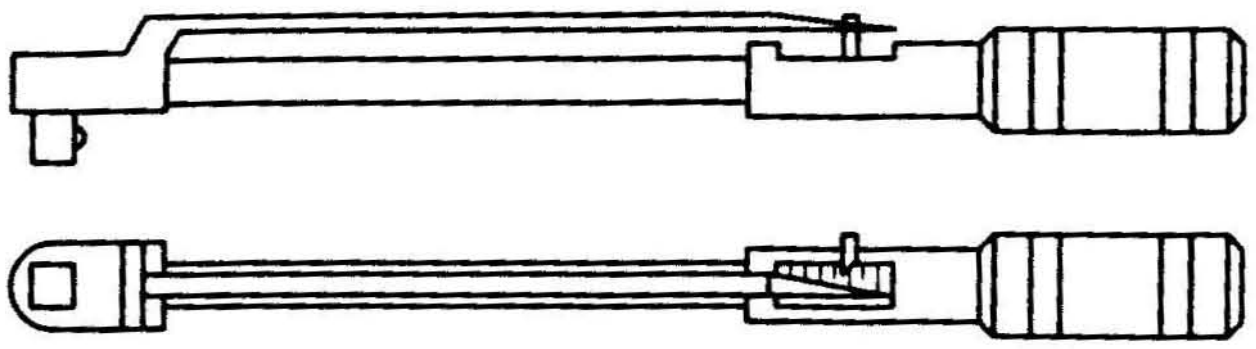

Figure B.7 — Class G: wrench flexion bar, adjustable, graduated

Bibliography

[1] ISO 1174-1, *Assembly tools for screws and nuts — Driving squares — Part 1: Driving squares for hand socket tools*

[2] ISO 1703:1983, *Assembly tools for screws and nuts — Nomenclature*

[3] ISO 9001, *Quality management systems — Requirements*

[4] *Fundamental standards — International vocabulary of basic and general terms in metrology (VIM).* BIPM, IEC, IFCC, ISO, IUPAC, IUPAP, OIML, 2nd edition, 1993

NATIONAL ANNEX A

(National Foreword)

A-1 BIS CERTIFICATION MARKING

The hand torque tools may also be marked with the Standard Mark.

The use of the Standard Mark is governed by the provisions of the *Bureau of Indian Standards Act*, 1986 and the Rules and Regulations made thereunder. The details of conditions under which the licence for the use of the Standard Mark may be granted to manufacturers or producers may be obtained from the Bureau of Indian Standards.

Bureau of Indian Standards

BIS is a statutory institution established under the *Bureau of Indian Standards Act*, 1986 to promote harmonious development of the activities of standardization, marking and quality certification of goods and attending to connected matters in the country.

Copyright

BIS has the copyright of all its publications. No part of these publications may be reproduced in any form without the prior permission in writing of BIS. This does not preclude the free use, in course of implementing the standard, of necessary details, such as symbols and sizes, type or grade designations. Enquiries relating to copyright be addressed to the Director (Publications), BIS.

Review of Indian Standards

Amendments are issued to standards as the need arises on the basis of comments. Standards are also reviewed periodically; a standard along with amendments is reaffirmed when such review indicates that no changes are needed; if the review indicates that changes are needed, it is taken up for revision. Users of Indian Standards should ascertain that they are in possession of the latest amendments or edition by referring to the latest issue of 'BIS Catalogue' and 'Standards: Monthly Additions'.

This Indian Standard has been developed from Doc: No. PGD/MGP 05 (539).

Amendments Issued Since Publication

Amendment No.	Date of Issue	Text Affected

BUREAU OF INDIAN STANDARDS

Headquarters:

Manak Bhavan, 9 Bahadur Shah Zafar Marg, New Delhi 110 002
Telephones: 2323 0131, 2323 3375, 2323 9402 *Website*: www.bis.org.in

Regional Offices:

		Telephones
Central :	Manak Bhavan, 9 Bahadur Shah Zafar Marg NEW DELHI 110 002	2323 7617 2323 3841
Eastern :	1/14, C.I.T. Scheme VII M, V.I.P. Road, Kankurgachi KOLKATA 700 054	2337 8499, 2337 8561 2337 8626, 2337 9120
Northern :	SCO 335-336, Sector 34-A, CHANDIGARH 160 022	260 3843 260 9285
Southern :	C.I.T. Campus, IV Cross Road, CHENNAI 600 113	2254 1216, 2254 1442 2254 2519, 2254 2315
Western :	Manakalaya, E9 MIDC, Marol, Andheri (East) MUMBAI 400 093	2832 9295, 2832 7858 2832 7891, 2832 7892

Branches: AHMEDABAD. BANGALORE. BHOPAL. BHUBANESHWAR. COIMBATORE. FARIDABAD. GHAZIABAD. GUWAHATI. HYDERABAD. JAIPUR. KANPUR. LUCKNOW. NAGPUR. PARWANOO. PATNA. PUNE. RAJKOT. THIRUVANANTHAPURAM. VISAKHAPATNAM.

Printed at Prabhat Offset Press, New Delhi-2